innoprot
cell based solutions

NOMAD CELL LINES

P70545-02R

Nomad Biosensors™ comprise a family of genetically encoded fluorescent sensors designed to monitor the signaling of G protein-coupled receptors (GPCRs) in cell-based assays.

Nomad Biosensors™ are engineered to measure the intracellular dynamics of second messengers such as calcium (Ca^{2+} Nomad), cAMP (cAMP Nomad), or diacylglycerol (DAG Nomad) upon GPCR activation. Additionally, β-arrestin signaling can also be studied using these biosensors. Nomad Biosensors™ can be combined in the same cell line for multiplex assays.

Prior to GPCR activation, the biosensors are localized in the plasma membrane. Upon ligand binding, the sensors undergo a conformational change that leads to an increase in fluorescence intensity and their relocalization within the vesicular trafficking pathways of the cells.

icAMPNOMAD M4

icAMP Assay

Product Name: icAMPNomad-M4 Receptor Cell Line
Reference: P70545-02R
Gene Name: Cholinergic receptor muscarinic 4 (M4)
cDNA Accession Number: X15265.1
Host Cell Line: U2OS
Selection Markers: Geneticin (G418) + Puromycin
Cell Quantity: > $3x10^6$ cells/vial
Storage Conditions: Liquid Nitrogen

About icAMPNomad-M4

Nomad cell lines are a reliable system for studying G protein-coupled receptor (GPCR) signaling in living cells.

Optimized for the integration into High Content Screening (HCS) and High Throughput Screening (HTS) workflows, icAMPNomad-M4 Receptor Cell Line stably express red icAMPNomad Biosensor along with the Cholinergic receptor muscarinic 4 (M4).

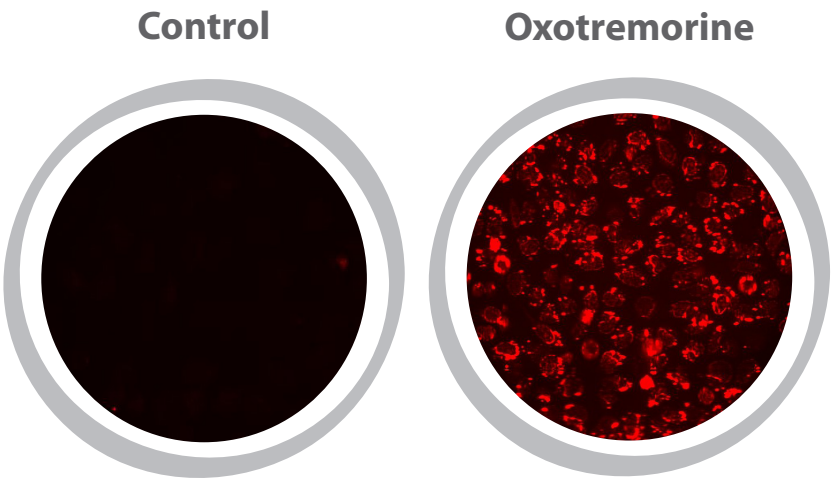

NOMAD CELL LINES

icAMP Agonism & Antagonism Assays

The icAMPNomad-M4 Receptor Cell Line was plated in a 96-well plate and incubated for a minimum of 4 hours and up to 24 hours at 37°C with 5% CO_2 to allow the cells to attach to the plate surface.

Agonism Assay: Cells were incubated with Oxotremorine diluted in a serum-reduced medium for 20–24 hours.

Antagonism Assay: Cells were incubated with atropine diluted in 300 nM oxotremorine serum-reduced medium for 20–24 hours.

The increase (Agonism Assay) or decrease (Antagonism Assay) in the fluorescence intensity of the red icAMPNomad biosensor (% Activity) was detected and analyzed using a microplate reader.

EC_{50} Oxotremorine: $4.27x10^{-8}$ M

Z´: 0.87+/- 0.01

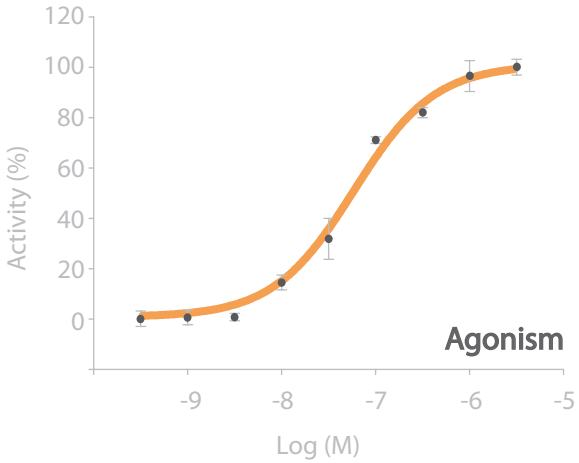

IC_{50} Atropine: $2.14x10^{-9}$ M

Z´: 0.96+/- 0.01

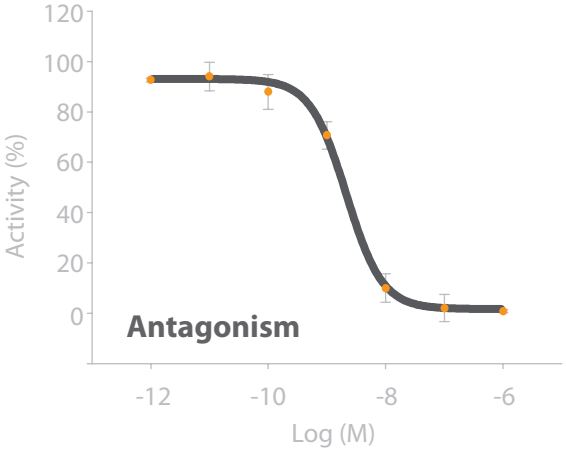

Figure 1. Dose-response curves for M4 ligands.
Top: *concentration response curve for oxotremorine in the agonism assay.*
Bottom: *concentration response curve for atropine for the antagonism assay.*
The % Activity corresponds to the fluorescence intensity emitted by the red icAMPNomad biosensor normalized against the controls.

INNOVATIVE TECHNOLOGIES IN BIOLOGICAL SYSTEMS, S.L.
Parque Tecnológico Bizkaia, Edificio 502, 1ª Planta | 48160 | Derio | Bizkaia
Tel.: +34 944005355 | Fax: +34 946579925
innoprot@innoprot.com | www.innoprot.com

innoprot cell based solutions